

**INSTALLATION INSTRUCTIONS**  
**PISTON / DIAPHRAGM INSTRUMENTS**  
**DIFFERENTIAL PRESSURE INSTRUMENTS**

For efficient working of your instrument, please read all instructions carefully before attempting to install.


**CAUTION :** Do not exceed maximum operating pressure given on the instrument label.

Check fluid compatibility with wetted parts before use.

**OPERATING PRINCIPLE**

Variations in pressure between high and low ports is sensed by a piston or diaphragm sensor (1) which moves in proportion to the pressure difference. A primary magnet (2) is attached to the sensor and moves with it in the same proportion. A SENSING ELEMENT rotary magnet (3) with pointer is magnetically coupled with the primary magnet, and is situated in an isolated cavity. Movement of rotary magnet with pointer indicates differential pressure on the dial.

Process fluids are isolated from dial case and switch enclosure.

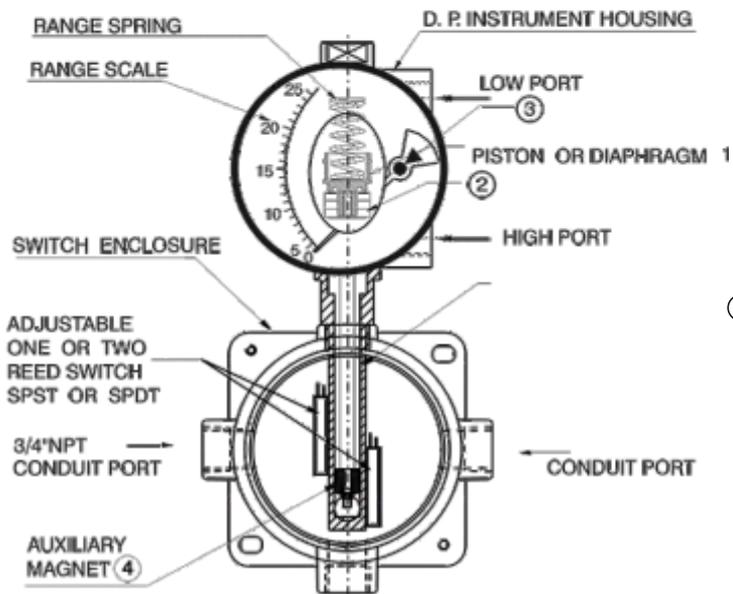

**PRECAUTIONS**

Do not connect "High" and "Low" ports to wrong pipe ends. Do not subject the instrument to excessive vibration.

The instrument is never to be used in an area where a magnetic field is present. It may show wrong readings.

As the instrument works on magnetic coupling, use only non magnetic fittings, parts etc. in areas closer than 50 mm on all sides, Otherwise calibration will get effected.

Do not try to open any part of the instrument for any reason, because if not reassembled properly calibration will be affected.

enclosure.

**SWITCH :**An auxiliary magnet (4) situated in the tube extension moves with the pressure sensors. Reed

switches mounted on the extension tube are activated 3/4" NPT due to interaction between switch contacts and field of auxiliary magnet. Switches can be adjusted to open or close at preset points.

**Note :** The instruments are calibrated to give  $\pm 2\%$  full scale accuracy on ascending readings.

## INSTALLATION

The instrument has entry ports at side. Depressurize the system and connect the high and low pressure lines of your system to the "High"  $\oplus$  & "Low"  $\ominus$  ports of the instrument, respectively.

It is recommended to use "O" rings with male connectors to avoid excessive tightening and to prevent leakage (For parallel threads). The instrument is now ready for operation.

Apply "High" and "Low" pressures simultaneously, to avoid damage to the internal parts.

If pressure exceeds the rated maximum pressure, "O" rings used on male connectors, and the teflon seal inside the pressure chamber of piston instrument will be damaged. In diaphragm instrument diaphragm may rupture. If maximum operating pressure is within the allowable limit, but

the differential pressure exceeds instrument range, properly there will be no damage to the instrument. Pointer

Form MKT:23/Ver 0

## SWITCH SETTING :

The switches are normally factory set to save time at customer's end. However they are field adjustable.

**CAUTION :** Supply should not exceed switch rating. For highersupply, use of relay circuit is recommended.

## SWITCH ADJUSTMENT

Unscrew the cover of electrical enclosure & keep it aside. Knurled head screws are provided at bottom for adjustment.

Rotate the screw anti-clockwise to increase the set point and clockwise to decrease the set point.

One or two trials may be necessary to attain the exact setpoint.

Above procedure to be followed by putting the instrument on test bed or while in actual service.



## SPST SWITCH

Switches are provided as per customer equipment. Please refer gauge label for switch specification.

### One SPST switch

Reed switches & terminal strip connection

### Two SPST switches

Reed switches & terminal strip connection

## SPDT SWITCH





Switches are provided as per customer equipment. Please refer gauge label for switch specification.

### One SPDT switch

Reed switches & terminal strip connection

### Two SPDT switches

Reed switches & terminal strip connection

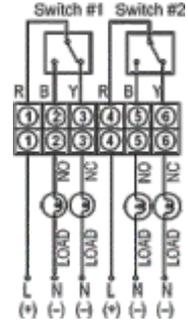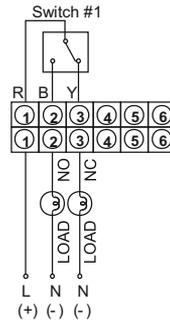

R=Red, B=Black, Y=Yellow, L=Live or +ve supply, N=Nutral or -ve supply

\* Body to be suitably earthed while using gauge + switch and only switch.

Authorised Dealer



*NK Instruments Pvt. Ltd.*

B-501/504, 5th floor, Raunak Arcade, Near THC Hospital, Gokhale Road, Naupada,  
Thane(W) 400602. Maharashtra INDIA      Telefax Nos.: 91-22-25301330 / 31 / 32  
E-Mail: sales@nkinstruments.com      Web: <http://www.nkinstruments.com>  
Skype: nitinkelkarskype      Gtalk: nkinstruments2006

